

iMAIL

LETTERS TO THE EDITOR

Artificial Intelligence-Based Assessment of Left Ventricular Filling Pressures From 2-Dimensional Cardiac Ultrasound Images



The estimation of left ventricular (LV) filling pressure from the ratio of transmitral and annular velocities (E/e') is used commonly for identifying diastolic dysfunction in patients who complain of exertional dyspnea (1). We have recently illustrated that LV and left atrial speckle tracking echocardiography (STE)-derived measurements have similar information content as do conventional 2-dimensional and Doppler methods for characterizing LV diastolic dysfunction (2). Therefore, an alternative approach could be to use an automated approach in which myocardial deformation variables with machine learning (ML) models deliver a rapid decision support system from just 2-dimensional cardiac ultrasound images for deriving the same level of information regarding left ventricular filling pressures (LVFP) as provided by E/e' .


We explored the development and validation of an ML model for assessing LVFP in 174 patients. The details regarding these subjects have been previously described (2). The study sample size was split into an ML training group of 130 patients (75%) and an ML testing group of 44 (25%) who also had the pulmonary capillary wedge pressure invasively measured using right cardiac catheterization. Patients were classified as elevated or reduced LVFP, as suggested by the echocardiographic ratio between early diastolic mitral flow velocities to early diastolic mitral annular velocity averaged from the septal and lateral positions (E/e') ≥ 13 . An ensemble model of ML algorithms was then applied to the STE data for the prediction of elevated LVFP. The models output in the testing sets were also verified for identification of elevated pulmonary capillary wedge pressure (≥ 18 mm Hg) (3).

Fourteen STE variables derived from parameters of the atrioventricular (AV) deformation, chamber volume, and volume expansion (Figure 1A) were used to build the ML model. The model was developed using a “majority voting” method combined from random forests, artificial neural networks, and support vector machines so that a patient was assigned the diagnosis of elevated LVFP if ≥ 2 ML models show this diagnosis (Figure 1B). To assess sample-induced bias and error rates; the final results are reported based on 10-fold cross-validation.

Feature relevance for STE parameters used in the ML algorithm was derived using information gain criterion and ranked using Ranker method (Figure 1A). Receiver-operating characteristic curves were compiled to evaluate the models. The overall accuracy of our model was based on area under the curve. Statistical analyses were performed using R: a language and environment for statistical computing (version 3.1.2, R Foundation, Vienna, Austria). ML algorithms and feature selection methods were implemented using R packages and Weka (open source software issued under the GNU General Public License).

Using the full set of STE features ($n = 14$), a 10-fold cross-validation showed a strong predictive ability of ML model for elevated LVFP (areas under the curve: training cohort = 0.847, testing cohort = 0.868). Based on the information gained, 11 features were found to best predict LVFP. Consistent with theoretical estimations, our ML models were found to perform better using this reduced set of features ($n = 11$), yielding areas under the curve of 0.853 and 0.881 for training and testing sets, respectively. In the testing set, the output defined as elevated LVFP as suggested by E/e' , was found to correctly identify 80% of patients with pulmonary capillary wedge pressure ≥ 18 mm Hg ($\kappa = 0.51$; $p < 0.001$).

Our work here is an extension of previous attempts of the application of ML to aid in the interpretation of cardiac imaging and clinically actionable phenotypic classifications (4). The use of automated STE analysis has been suggested to improve reproducibility (5). Our data further suggests that noninvasive assessment of LVFP using STE is feasible and suggests a method that can be used to accommodate the large amount of parameters found within the STE data for enhancement of the currently used methods. In the future, it would be worthwhile to assess whether such a decision support system can be used to completely fulfill all the steps recommended currently in guideline documents for assessing diastolic function (1). Development of such automated algorithms may be significant in the setting of the growing burden of cardiovascular disease in the community, the increased costs of sophisticated diagnostics, and the projected workforce shortage in the field. Finally, it is important to note that, while our model was developed based on E/e' , this Doppler-based method is known to have some limitations (1). A direct comparison between our STE-based model and E/e' against directly measured pressures is required to test the potential ability of STE to overcome such limitations.

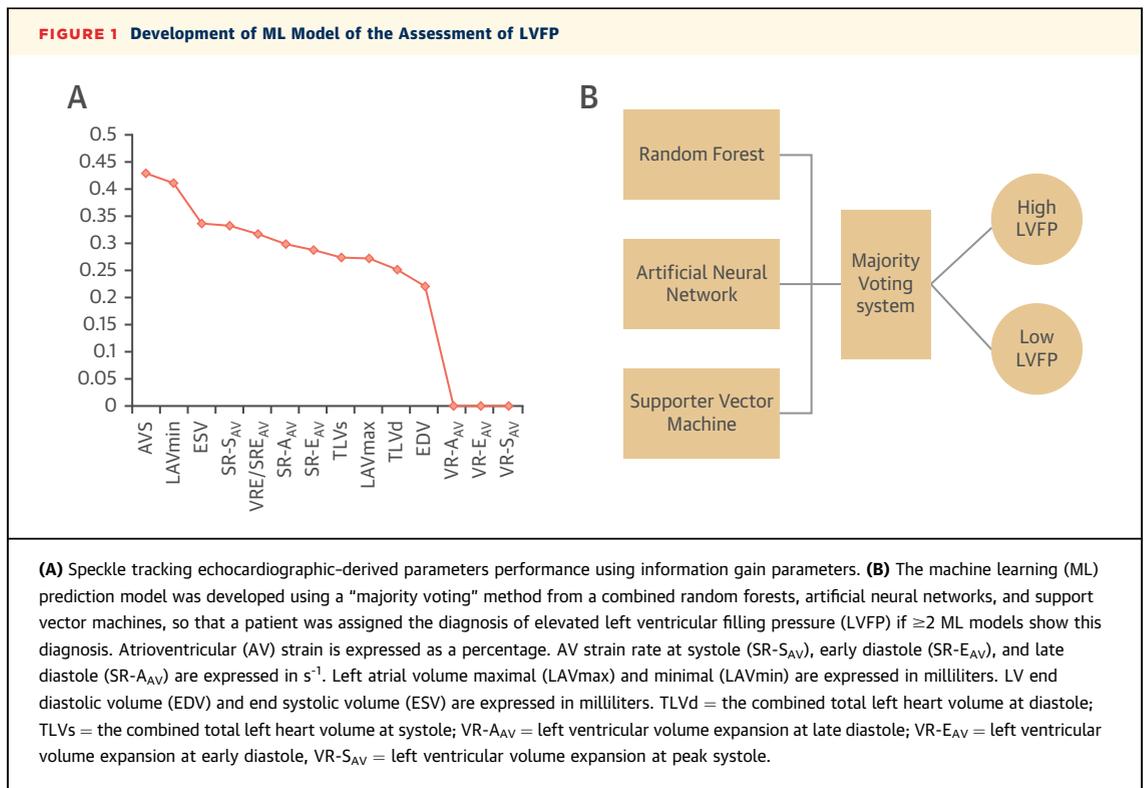

Alaa Mabrouk Salem Omar, MD, PhD

Khader Shameer, PhD

Sukrit Narula, BS

Mohamed Ahmed Abdel Rahman, MD

Osama Rifaie, MD

Jagat Narula, MD, PhD

Joel T. Dudley, PhD

Partho P. Sengupta, MD, DM*

*Icahn School of Medicine at Mount Sinai, New York

Mount Sinai Medical Center

One Gustave L. Levy Place, P.O. Box 1030

New York, New York 10029

E-mail: Partho.Sengupta@wvumedicine.org

<https://doi.org/10.1016/j.jcmg.2017.05.003>

© 2018 by the American College of Cardiology Foundation. Published by Elsevier.

Please note: Dr. Dudley has received consulting fees or honoraria from Janssen Pharmaceuticals, GlaxoSmithKline, AstraZeneca, and Hoffman-La Roche; is a scientific advisor to LAM Therapeutics; and holds equity in NuMedii Inc., Ayasdi Inc., and Ontomics, Inc. Dr. Sengupta has received research grants from Heart Test Lab and Echo Sense; and consulting fees from Intel and Heart Test Lab. All other authors have reported that they have no relationships relevant to the contents of this paper to disclose. Theodore Abraham, MD, served as the Guest Editor for this paper. Drs. Omar and Shameer contributed equally to this work.

REFERENCES

1. Nagueh SF, Smiseth OA, Appleton CP, et al. Recommendations for the evaluation of left ventricular diastolic function by echocardiography: an update from the American Society of Echocardiography and the European Association of Cardiovascular Imaging. *J Am Soc Echocardiogr* 2016;29:277-314.

2. Omar AM, Narula S, Abdel Rahman MA, et al. Precision phenotyping in heart failure and pattern clustering of ultrasound data for the assessment of diastolic dysfunction. *J Am Coll Cardiol Img* 2017;10:1291-303.

3. Forrester JS, Diamond G, Chatterjee K, Swan HJ. Medical therapy of acute myocardial infarction by application of hemodynamic subsets (second of two parts). *N Engl J Med* 1976;295:1404-13.

4. Narula S, Shameer K, Salem Omar A, Dudley JT, Sengupta PP. Machine-learning algorithms to automate morphological and functional assessments in 2D echocardiography. *J Am Coll Cardiol* 2016;68:2287-95.

5. Knackstedt C, Bekkers SC, Schummers G, et al. Fully automated versus standard tracking of left ventricular ejection fraction and longitudinal strain: the FAST-EFs Multicenter Study. *J Am Coll Cardiol* 2015;66:1456-66.

The Normal Mitral Valve Annulus in Humans Defined Using 3-Dimensional Transesophageal Echocardiography



Mitral regurgitation is the most common valvular lesion in Europe, frequently assessed with transesophageal and transthoracic echocardiography (TEE/TTE). The spatial resolution of 3-dimensional (3D) TEE is excellent and facilitates measurements similar to those made under direct visualization of the valve (1). A range of reference values for the normal mitral valve annulus (MVA) are essential for clinical practice; whereas normal reference ranges have been established using 3D TTE (2), there is minimal data in the published reports for 3D TEE.